



HODO KN95 Protective Masks



Product Description



KN95 Masks Fold in Half 3-D Design

PFE \geq 95%

3-D Design



Invisible Nose Bridge



Elastic Ear Rope



Soft & Comfortable





4-Ply Protection Filtration

Anti-Virus, Safe, Protection, Soft

(First Layer) PP No-woven Fabric

Isolate large Particles
Block liquid

Forth Layer PP No-woven Fabric


Soft-skin, Reduce skin
irritation and
bacterial invasion

Filter Fine particles
(PM2.5)

(Second Layer) Electrostatic cotton

(Third Layer) BFE99 Melted Fabric

Adsorb bacteria 3
microns BFE \geq 99%

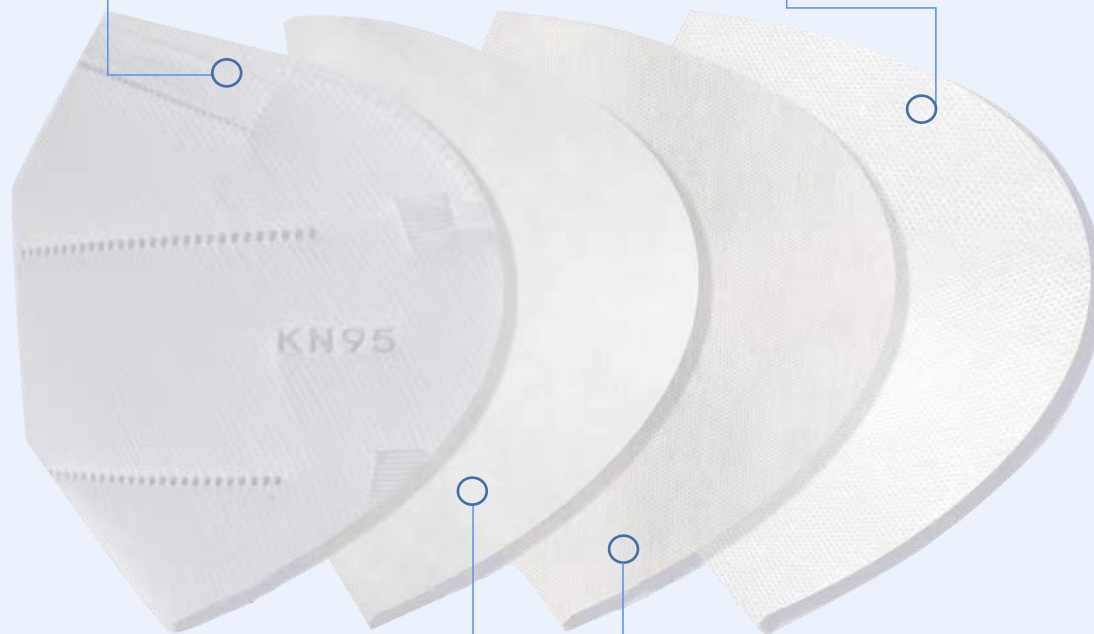

Close skin soft stick a face, Breathable

Flexible Adjustable



Front



Opposite

Shelf life : 3 years

Size : 15.5×10cm

Color : White ○

Workshop

Automatic mask production line



Packing



Certificates

شهادة - 증명서 - Certificat - 證明書 - Сертификат - Certificate

Form QAT_10-M04, version 00, effective since March 6th, 2020

Certificate of Compliance

No. 0B200319.JFEUS97

Certificate's Holder:

Certification ECM Mark:

Product: Filtered anti-particle mask
Model(s): KN95
Classification: 9001 FFP2 NR D
Verification to: Standard: EN 149:2001+A1:2009
related to CE Directive(s): R 2016/425 (Personal Protective Equipment)

Remark: This document has been issued on a voluntary basis and upon request of the manufacturer. It is our opinion that the technical documentation received from the manufacturer is satisfactory for the requirements of the ECM Certification Mark. The conformity mark above can be affixed on the products accordingly to the ECM regulation about its release and its use.

Additional information and clarification about the Marking:

CE The manufacturer is responsible for the CE Marking process. This document has been issued on the basis of the regulation on ECM Voluntary Mark for the certification of products. RG01_ECM rev.3 available at: www.entecerma.it

Issuance date: 19 March 2020
Expiry date: 18 March 2025

Reviewer
Technical expert
Amanda Payne

Approver
ECM Service Director
Luca Bedonni

Ente Certificazione Macchine Srl
Via Ca' Bella, 243 - Loc. Castello di Serravalle - 40053 Valsamoggia (BO) - ITALY
+39 051 6705141 +39 051 6705156 info@entecerma.it www.entecerma.it



Test Report

Product Name: KN95 Masks
Applicant :
Manufacturer:
Test Type: Consignation Testing



Test Report

Product Name	KN95 Masks	Specification	_____
		Brand	_____
Applicant	_____	Tel	_____
Manufacturer	_____	Sample grade	KN95
Sample quantity	29 PCS	Sample date	15 th . Mar, 2020
Test Type	Consignment Testing	Article number/Batch number/Style number	---
Sample sate	Meet inspection requirements		
Test standards	GB 2626-2006		
Test conclusion	The samples were inspected and the inspected items met the KN95 level requirements specified in the GB2626-2006 standard		
Notes	This report is only responsible for incoming samples		

Approver: 陳敏

Reviewer: 姚永清

Main inspector: 蔡煥文

Number	Test Item	Unit	Technical Requirement	Test Result				Single Item Decision
1	Respiratory resistance	Pa	The total inspiratory resistance of each sample should not be greater than 350, and the total expiratory resistance should be greater than 250	Sample No		Measured value		Pass
				Expiratory resistance	Not processed	1#	124.1	
						2#	133.2	
					processed	3#	129.6	
						4#	136.7	
				Inhalation resistance	Not processed	5#	170.8	
						6#	153.8	
					processed	7#	167.4	
						8#	172.3	
				2	Filtration efficiency (%) (NaCl particulates)	— —	KN90: ≥90.0 KN95: ≥95.0 KN100: ≥99.97	
Not preprocessed	9#	98.8						
	10#	98.5						
	11#	99.2						
	12#	98.5						
	13#	98.6						
	14#	98.7						
	15#	98.9						
	16#	98.5						
preprocessed	17#	98.6						
	18#	98.0						
	19#	98.4						
	20#	98.0						
	21#	98.3						
	22#	98.5						
	23#	98.4						